



Instrument Control

Start Estimated Time Remaining (hh:mm):

Stop

Disconnect Status:

Extend...

Temperature

Sample: Heat Sink:

Cover: Block:


Cycle

Stage: Rep:

Time (mm:ss): Step:

State:

Thermal Cycler Protocol

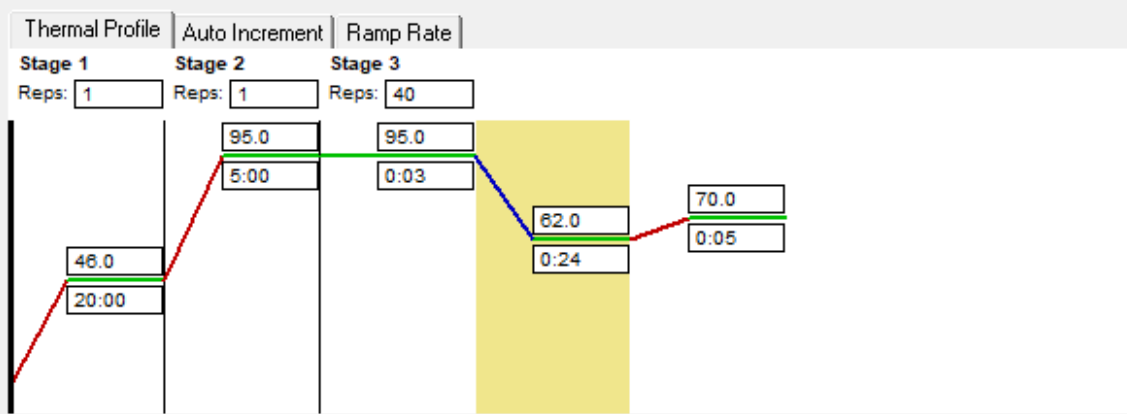

Add Cycle Add Hold Add Step Add Dissociation Stage Delete Help

Settings

Sample Volume (µL): 20

Run Mode: Fast 7500 Expert Mode [Select/View Filters...](#)

Data Collection: Stage 3, Step 2 (62.0 @ 0:24)